



the difference is clear

Summary Sheet

Product Type	Quantity
Aneroid/Mercurial Blood Pressure Monitor	6
Cautery	1
Couch	1
Digital blood Pressure Monitor	18
Diagnostic Set	3
Ear Syringe	1
ECG	1
Height Measure	5
Nebuliser	1
Pulse Oximeter	1
Scales	13
Spirometer	4
Thermometer	5
Ultrasound (Fetal Dopplex)	2
Vaccine Fridge	8



the difference is clear

Certificate of Compliance

Client The Medical centre

Equipment Details

Type	Aneroid Sphygmomanometer
Manufacturer	Riester
Model	
Serial Number	HMC 2


The following accuracy and performance checks were carried out in accordance with manufacturer's guidelines and procedures laid down by Vitalograph Ltd.

Test Results

Visual inspection	Pass
Static Pressure Test	Pass
Leak Test	Pass
Functionality Test	Pass

Comments:

Signed:

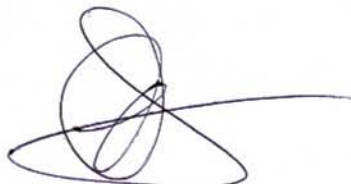

Name: Wilkinson

Test Date: 28/09/07



the difference is clear

Certificate of Compliance

Client The Medical Centre

Equipment Details

Type	Pulse Oximeter
Manufacturer	BCI
Model	3301
Serial Number	170268506

The following accuracy and performance checks were carried out in accordance with manufacturer's guidelines and procedures laid down by Vitalograph Ltd.

Test Results

Visual inspection	Pass
SPO2 Test	Pass
Functionality Test	Pass

Comments:

Signed:

Name: Wilkinson

Test Date: 28/09/2007





the difference is clear

Certificate of Compliance

Client The Medical Centre

Equipment Details

Type	ECG Machine
Manufacturer	Seca
Model	
Serial Number	02257


The following accuracy and performance checks were carried out in accordance with manufacturer's guidelines and procedures laid down by Vitalograph Ltd.

Test Results

Visual inspection	Pass
Simulation Tests	Pass
Electrical Safety Test	Pass
Functionality Test	Pass

Comments:

Signed:



Name: Wilkinson

Test Date: 28/09/ 2007



Certificate of Compliance

Client The Medical Centre

Equipment Details

Type	Spirometer
Manufacturer	Micro Medical
Model	Micro loop
Serial Number	HMC 4

The following accuracy and performance checks were carried out in accordance with manufacturer's guidelines and procedures laid down by Vitalograph Ltd.

Test Results

Visual inspection	Pass
Volume Measurement Accuracy +/- 3%	Pass
Electrical Safety Test	Pass
Functionality Test	Pass

Comments:

Signed:

Name: Wilkinson

Test Date: 28/09/2007